

# Trabecular Metal™ Dental Implants: Overview of design and developmental research

Michael Collins, MSBME, MBA,\* Jeff Bassett, BS,† Hai Bo Wen, PhD,‡ Chris Gervais, BS,€ Matt Lomicka, MS,£ Savvas Papanicolaou, MS¥

\* Vice President, Research, Development and Education

† Director, Engineering

‡ Associate Director, Dental Research and Clinical Affairs

€ Associate Director, Engineering

£ Senior Design Engineer

¥ Design Engineer


## Abstract

Research in implant biomaterials and surface technologies over the past three decades has led to development of a porous tantalum biomaterial with a structure and elasticity similar to trabecular bone. This material has been used extensively in orthopedic reconstructions for over a decade. Recent advancements have led to the development of a new *Trabecular Metal* Dental Implant (Zimmer Dental Inc., Carlsbad, CA, USA). This article presents an overview of the implant design, and discusses some of the underlying research that led to its development.

## Introduction


Attempts to replace missing teeth with implanted materials have been observed in ancient human remains,<sup>1</sup> and documented experimentally and clinically in the dental literature since the 19<sup>th</sup> century.<sup>2-3</sup> Over the past 3 decades, dental implant systems have been commercialized in a variety of materials, including tantalum,<sup>2,4-5</sup> vitreous carbon,<sup>6-8</sup> single-crystal sapphire,<sup>9-10</sup> stainless steel,<sup>2,3</sup> titanium,<sup>3,11-14</sup> and other substances. The era of modern implant dentistry, however, is primarily built on orthopedic titanium research subsequently adapted for dental implant applications. In 1940, orthopedic surgeons<sup>15</sup> first experimented with the surgical use of titanium and reported its extreme biocompatibility. In the 1950s, other orthopedic surgeons<sup>16-17</sup> documented titanium's superior ability to withstand corrosion and remain relatively inert in the body.<sup>18-20</sup> In 1977, orthopedic surgeon Per-Ingvar Brånemark and colleagues<sup>11-14</sup> published results of their monumental 10-year dental implant study. The Brånemark team documented<sup>11-14</sup> the processes and conditions in which ordered, living bone could form a direct structural and functional connection with a load-carrying titanium dental implant. The researchers<sup>11</sup> coined the term "osseointegration" to describe the natural phenomenon first reported more than three decades earlier by their predecessors.<sup>15-17</sup>

In the three decades since the seminal Brånemark study<sup>11</sup> was published, continuing dental and orthopedic research has focused on various techniques for enhancing bone apposition to implanted titanium surfaces. Despite differences in anatomical locations and bone structures, a variety of surface modification techniques developed in orthopedics have since been successfully adapted for dental implant use. Among these are hydroxylapatite (HA), titanium plasma spray (TPS), and porous surface coatings, such as porous bead surfaces and cancellous-structured titanium (CSTi™) Coating.

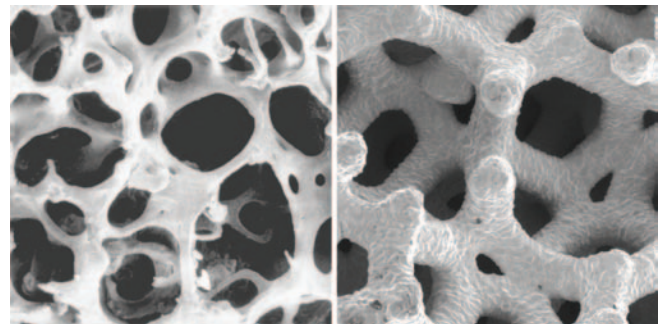

**Figure 1.** SEM view of trabecular bone (left) and Trabecular Metal Material (right).

*Trabecular Metal* Material (Zimmer Dental Inc., Carlsbad, CA, USA) is a porous biomaterial with a structure and stiffness similar to trabecular bone (**Figure 1**).<sup>21-26</sup> It is fabricated by coating a vitreous carbon skeleton with tantalum (**Figure 2**) through a proprietary chemical vapor deposition coating process. The tantalum exhibits a crystallographic growth pattern<sup>26-27</sup> on the vitreous carbon surface of the interconnecting struts<sup>23,27-31</sup> (**Figure 1**) that form the material. *Trabecular Metal* Technology significantly differs from sintered bead surfaces, titanium plasma-sprayed surfaces, titanium fiber mesh and titanium foam in the high degree of its interconnected porosity (up to 80%) and the regularity of its pore size and shape.<sup>23,27-28,30-31</sup> In contrast to conventional bone-to-implant contact achieved by non-porous surfaces, *Trabecular Metal* Technology's geometrical network of interconnected pores is designed for biological ingrowth through the pores.<sup>20,24-27,30-32</sup> This *Trabecular Metal* Material has been used extensively in orthopedic reconstructions for more than a decade.<sup>23-25,28,31,33-34</sup> The present article will present an overview of a new *Trabecular Metal* Dental Implant and its developmental research.

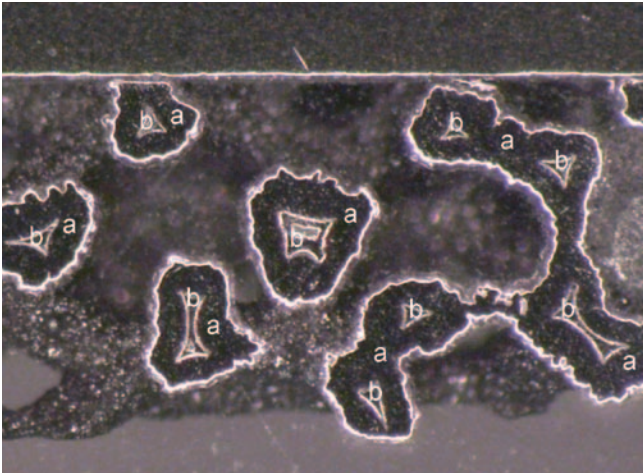

**Figure 2.** SEM cross-section of Trabecular Metal Material struts shows the (a) tantalum coating over (b) the vitreous carbon skeleton.

### Preliminary experiments with Trabecular Metal Technology as a biomaterial


Trabecular Metal Technology was originally commercialized as *Hedrocel*<sup>®</sup> Material, and envisioned as a 3-dimensional bone augmentation material. Commencing in the early 1990s, a series of *in vivo* canine evaluations<sup>30,35-37</sup> in the canine model and mechanical testing<sup>38</sup> experimentally evaluated Trabecular Metal Material's 3-dimensional, open-cell structure as a potential implant for cancellous bone ingrowth and support of a dental implant in the alveolar ridge.

**National Institutes of Health Research Grant (DE09781)** Under a research grant from the National Institutes of Health, Kaplan et al.<sup>30,35-37</sup> created 18mm, full-thickness mandibular resections from the right hemi-mandibles of 6 dogs. A Trabecular Metal Implant was placed in the site and stabilized with a 10-hole reconstruction plate.<sup>30,35-37</sup> In the left (opposite) hemi-mandibles, a 17mm, full-thickness resection was made and then augmented with the bone resected from the right side of the jaw, and stabilized with a 10-hole reconstruction plate.<sup>30,35-37</sup> Animals were subjected to daily examination and monthly ventrodorsal radiographs for a period of 6 months to assess healing of the defect sites.<sup>30,35-37</sup>


Reconstruction plates were removed after 3 months in animals that exhibited mandibular stability in radiographic and physical examinations.<sup>30,35-37</sup> Animals that did not demonstrate stability after 3 months were allowed to continue healing and monthly evaluations until stability was confirmed and the plate could be removed.<sup>30,35-37</sup> After 6 months, all dogs were sacrificed and the entire mandible was harvested from each animal.<sup>30,35-37</sup> Any remaining compression plates were removed from the dogs at the time of sacrifice.<sup>30,35-37</sup> Each mandible was sectioned in left (control group) and right (test group) halves.<sup>30,35-37</sup> Mandible halves were then sectioned and prepared for histologic analysis.<sup>30,35-37</sup>

A total of 6 mandibles were obtained.<sup>30,35-37</sup> In 2 of these, the test implant had fallen out secondary to resorption of the adjacent bone caused by infection.<sup>30,35-37</sup> In all surviving samples, the Trabecular Metal Material side was compared with the contralateral control side.<sup>30,35-37</sup> All 4 surviving samples had osteoid crossing through the Trabecular Metal Implant, and 3 out of 4 samples had mineralized bone in the center of the material (Figure 3).<sup>30,35-37</sup> One sample had mineralized bone at the edges, but the center was not yet mineralized (Figures 4 and 5).<sup>30,35-37</sup> The majority of the mineralization appeared at the edges of the (osteotomy) cut.<sup>30,35-37</sup> There seemed to be more bone forming at the caudal, superior and the lingual aspects of the implants as opposed to the cranial, inferior and buccal sides.<sup>30,35-37</sup>

Most of the new bone was woven (Figure 4), however small foci of lamellar bone were seen mostly at the edges of the implant bone interface.<sup>30,35-37</sup> Marrow elements were not seen in any sample.<sup>36</sup> Cellular elements (osteoblasts) were identified in the woven bone in the implant; however, these were quantitatively more prevalent at the edges.<sup>30,35-37</sup>

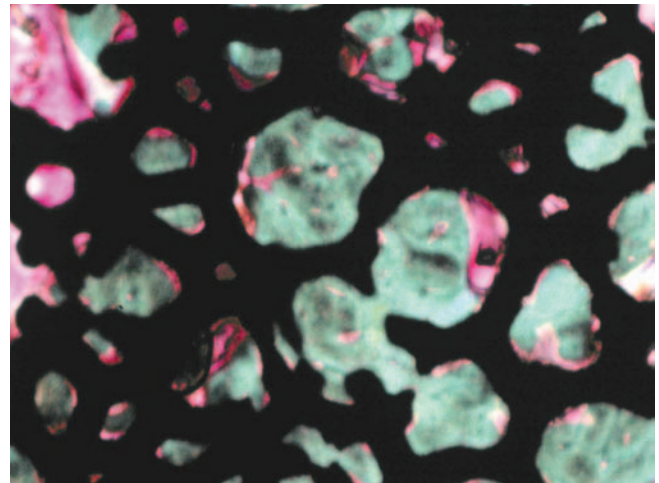


**Figure 3.** Mineralized bone ingrowth into porous Trabecular Metal Material (seen as black in the photograph).<sup>37</sup> Osteoid matrix conversion to mineralized bone is shown<sup>37</sup> (MIBS stain).

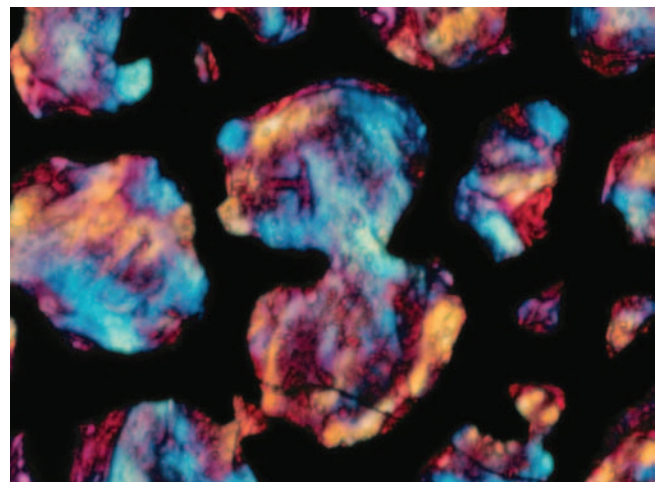

**Figure 4.** Woven bone ingrowth into Trabecular Metal Material pores<sup>37</sup> (trichrome stain, semi-polarized light).



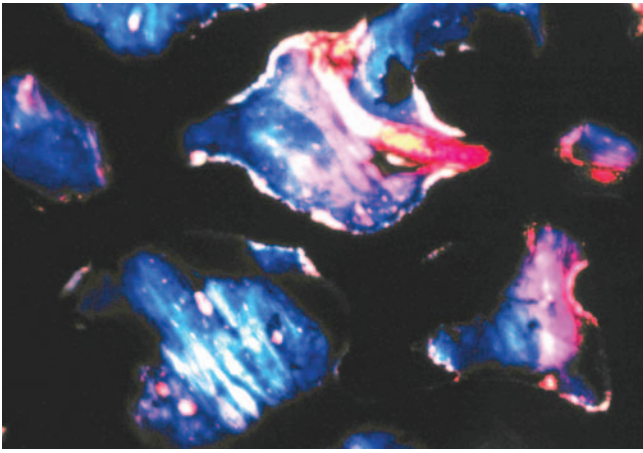

**Figure 5.** Lamellar bone formation inside porous Trabecular Metal Material.<sup>37</sup> According to the researchers, “the maturation of woven bone into lamellar bone is indicative of normal bone and permanency”<sup>37</sup> (trichrome stain, semi-polarized light).

Control samples exhibited good evidence of union in all cases, including the cases that were infected.<sup>30,35-37</sup> In comparison to the control cases, the 4 surviving test samples exhibited greater new bone formation in 1 case, less new bone formation in 1 case, and more area of bone formation in 2 cases, but the degree of mineralization was slightly less than that of the control samples.<sup>30,35-37</sup> The researchers<sup>30,35-37</sup> concluded that *Trabecular Metal* Technology and autogenous bone were equally successful in treating mandibular discontinuity defects. Bone grew into *Trabecular Metal* Material, mineralized and developed cellular components.<sup>30,35-37</sup>

#### United States Patent No. 5,282,861 Issued in 1994

The inventor of United States Patent No. 5,282,861 was also involved in research conducted under the *National Institutes of Health Research Grant (DE09781-03)* cited above.<sup>35</sup> This patent stated that *Trabecular Metal* Technology could be potentially used for “alveolar ridge augmentation, periodontics, and orthognathic reconstruction,” and that it was “useful in orthopedic applications as well.” Although *Trabecular Metal* Technology’s actual commercialization has been strictly limited to orthopedic applications to date, the 1994 patent (U.S. 5,282,861) further stated that the “present invention may also be used for tooth replacement because of the ability to induce tissue and bone growth even in the face of mildly infectious conditions. For example, an artificial tooth can be joined to an open cell tantalum stem and positioned in an appropriately sized hole in the jaw. The gum is allowed to rest against the artificial tooth and some of the stem to form a seal.” While this proposed dental implant design was never developed with *Trabecular Metal* Material a similar design made with titanium fiber mesh had been previously launched during the 1970s, but the fibro-osseous interface that it developed limited its success.<sup>39-46</sup>

#### Mechanical integrity between Trabecular Metal Material and a single-tooth implant

Dillion et al.<sup>38</sup> conducted a mechanical experiment to determine the ability of a 3-dimensional *Trabecular Metal* Material bone graft to support an implant-supported, single-tooth restoration.

A 3.7mm-diameter threaded titanium implant (*Screw-Vent*<sup>®</sup> Implant, Zimmer Dental Inc.) was placed in a 10mm x 20mm x 25mm *Trabecular Metal* Material porous tantalum block, which was currently under investigation for use as a bone substitute for large segmental defects.<sup>38</sup> The system was evaluated in single-cycle and fatigue in axial compression and cantilever bending. Compression samples were loaded at 25N/sec in air to a maximum of 300N, and bending samples were loaded at 25N/sec in air to failure.<sup>38</sup> Fatigue samples were tested in Ringers at 37°C at 5Hz to  $2.5 \times 10^6$  cycles.<sup>38</sup> Compressive fatigue failure was defined as 0.03mm of permanent deformation.<sup>38</sup> Results showed a mean single-cycle bending strength of  $1.04 \pm 0.13$ kN-mm and a mean displacement of  $2.47 \pm 0.61$ mm using a lever arm of 7.5mm.<sup>38</sup> Axial compression tests showed a mean displacement of  $0.17 \pm 0.01$ mm at the maximum 300N load and the average load value at which the sample began to yield was 0.07kN ( $\pm .028$ kN).<sup>38</sup> A cantilever bending S/N curve was generated from 80% of yield to run-out at  $2.5 \times 10^6$  cycles.<sup>38</sup> No failure of the *Trabecular Metal* Material or at the interface was detected.<sup>38</sup> All samples failed due to deformation of the abutment screw.<sup>38</sup> Axial compressive fatigue was performed to a maximum load of 600N, which was approximately four times normal biting force with no failure.<sup>38</sup> Both single-cycle and fatigue tests indicated that the implant/*Trabecular Metal* Material system was able to withstand loads that were significantly greater than those found *in vivo*.<sup>38</sup> Failure of the system occurred in the screw attaching the abutment rather than at the implant/*Trabecular Metal* Material interface or within the *Trabecular Metal* Material itself.<sup>38</sup>

**Mechanical feasibility study on the potential use of Trabecular Metal Technology as a dental implant material (ZRR-ZD-00011-07)** Cylindrical and hexagonal blocks of *Trabecular Metal* Material were evaluated for push-in/push-out force, removal torque, and static compression evaluations in a polyether polyurethane surrogate bone material to determine how the material might function during placement into bone, and how it might withstand direct loading. Large-diameter (6.0mm) *Trabecular Metal* Material blocks showed good initial stability and were strong enough to resist compressive loading forces that exceeded those documented for the oral environment. Smaller diameter (3.7mm, 3.0mm) *Trabecular Metal* Material blocks would benefit from an anti-rotational feature, such as external threads, to improve initial stability and internal reinforcement to resist compressive forces in the oral environment. For example, an implant made of both titanium and *Trabecular Metal* Material would be significantly stronger than solid *Trabecular Metal* Material blocks alone. Results from these experiments indicate that a combination of *Trabecular Metal* Material and titanium will provide acceptable mechanical characteristics for a dental implant.

#### Development of Trabecular Metal Technology as a dental implant

The implant is a tapered, multi-threaded, endosseous design similar to its predicate, the *Tapered Screw-Vent*<sup>®</sup> Implant (Zimmer Dental Inc.), but modified with a

*Trabecular Metal* Material midsection (**Figure 6**). The coronal, apical and internal implant structures are made of titanium alloy (Ti-6Al-4V grade 5) with a microtextured surface created by grit-blasting with hydroxylapatite (*MTX*<sup>®</sup> Surface). The coronal section features cervical micro-grooves and Zimmer Dental's internal hex, friction-fit connection, and the apical section features self-tapping threads. In the midsection of the implant, the *Trabecular Metal* Material is made of tantalum (98%) over a vitreous carbon substrate (2%) (**Figure 2**).



**Figure 6.** Trabecular Metal Dental Implant.

**Tantalum** This highly biocompatible<sup>47-49</sup> metal has been widely used for over half a century in implanted medical devices for humans: dental implants,<sup>2,4-5</sup> orthopedic implants,<sup>24-26,29,32-34,49-50</sup> surgical ligation clips,<sup>47,51</sup> plates, nets and wires used in neurosurgery, cranioplasty, and oral and maxillofacial reconstructions,<sup>47,52-56</sup> electrodes for pacemakers,<sup>47,57</sup> and many other clinical applications.<sup>47,58-59</sup> It has been reported that tantalum does not elicit the cytotoxicity levels associated with some other metals, such as nickel, cobalt and chromium,<sup>47,60</sup> and that it exhibits strong resistance to oxidation, corrosion and concomitant ion production.<sup>47,41,60-63</sup> Tantalum was initially Brånemark's<sup>13</sup> biomaterial of choice for his early bone growth research. The high cost of tantalum, however, made titanium a more feasible material at the time.

**Vitreous carbon** One early clinical concern in the development of a *Trabecular Metal* Implant was the effect that exposure of its internal vitreous carbon core

(**Figure 2**) might have in the osseous environment. Long-term use as a dental implant material in humans,<sup>6-8</sup> and short-<sup>64-65</sup> and long-term<sup>66</sup> animal studies have demonstrated that vitreous carbon is well-tolerated in the oral environment.<sup>6</sup> A five-year systemic, toxicological, carcinogenic study in dogs reported that vitreous carbon implants exhibited no systemic responses in the major organs, tissues, blood or urine, and no evidence of inflammatory response or foreign body reactions in the adjacent tissues.<sup>6,66</sup> Large-scale hard- and soft-tissue ingrowth into the macroscopic grooves and other surface architecture of vitreous carbon has been extensively documented.<sup>6,67-68</sup>

**Mechanical evaluation of 4.7mm-diameter Trabecular Metal Dental Implants (ZRR-ZD-00065-00)** The purpose of this experiment was to determine if *Trabecular Metal* Implants would exhibit an adequate fatigue endurance limit that was equal to or greater than 90 lbs (400N), when subjected to cyclic compressive loading. This strength limitation was based on expected bite force ranges reported in the molar region.<sup>69</sup> Other important data collected for investigative purposes included ultimate strength during static compression loading and failure modes under static and fatigue loading. Evaluations were performed with *Trabecular Metal* Dental Implants, 4.7mm in diameter, in accordance with corporate requirements (ZRP-ZD-00065-00 and TP-307, Zimmer Dental Inc.), good manufacturing practices, and international standards.<sup>70</sup> The 4.7mm diameter *Trabecular Metal* Implants had an endurance limit of 100 lbs (445N); therefore, it was concluded that both the 4.7mm and 6.0mm diameter *Trabecular Metal* Implants could withstand the forces anticipated in the molar region.

**Abrasion evaluations of dental implants with porous surfaces (ZRM-ZD-00028-00)** This experiment was conducted to evaluate whether the friction caused by implant placement into an osteotomy was capable of damaging porous implant surfaces. Implants with two different porous surfaces were evaluated: *Trabecular Metal* Dental Implants and Cancellous-Structured Titanium (*CSTi*) dental implants. Test samples were microscopically examined at various magnifications, and compared before and after placement into two substrates: a synthetic surrogate bone material made of rigid, polyether polyurethane with a fine, closed-cell structure (density = 0.32g/cm<sup>3</sup>; 20 lb/ft<sup>3</sup>) (Last-A-Foam<sup>®</sup>, General Plastics Manufacturing Co., Tacoma, WA) (bone foam) and bovine condyle. Abrasion leading to subsequent release of metal debris from the implant surfaces was not expected because of differences in shear strengths between porous metal implants and bone. In this study, the *Trabecular Metal* Material and *CSTi* dental implants showed no evidence of abrasion or subsequent release of metal debris into the osteotomy. This was identified under 24X magnification, and was more evident under 65X and 137X magnification levels, where porous sections oriented both parallel and perpendicular to the long axis of the implants showed no deformation after implant placement.

**Insertion torque analysis of Zimmer Trabecular Metal Dental Implants in simulated dense bone (ZRR-ZD-00060-00 Add 1, ZRM-ZD-00034-00, ZRR-ZD-00098-00, ZRR-ZD-00060-00 Add 3)** Implant insertion torque values for *Trabecular Metal* Technology test implants and 2 titanium control implants (*Tapered Screw-Vent* Implant, Zimmer Dental Inc.; NobelReplace,<sup>®</sup> Nobel Biocare Implant, Yorba Linda, CA) were evaluated in bone foam. The composition of the bone foam consisted of a dense outer layer (50 lb/ft<sup>3</sup>) analogous to cortical bone, and a solid, rigid foam core (30 lb/ft<sup>3</sup>) analogous to trabecular bone. This experiment was conducted to determine if the insertion torque required to place the *Trabecular Metal* Implant in simulated dense bone was comparable to that of the control implants. The *Tapered Screw-Vent* Implant<sup>71-72</sup> and NobelReplace<sup>73-74</sup> implants were selected as controls because of their high documented success rates under delayed and immediate loading conditions. Control implant insertion torque values ranged from a maximum of 186.5Ncm (average = 157.9 ± 21.2Ncm) (*Tapered Screw-Vent*, 6.0mm x 13mm) to a minimum of 84.5Ncm (average = 89.5 ± 3.9Ncm) (NobelReplace Implant, 5.0mm x 13mm) (**Table 1**).

In a preliminary insertion torque experiment, insertion torque values were recorded for both implants in the same simulated bone model. *Tapered Screw-Vent* Implants (6.0mm x 13mm) exhibited significantly higher insertion torque values than NobelReplace implants (5.0mm x 13mm). These implants were selected as control implants in the present study because they represented a theoretical range of highest and lowest acceptable insertion torque values, respectively. *Trabecular Metal* test implants (6.0mm x 13mm and 4.7mm x 13mm) approximated the dimensions of the control implants. Acceptance criteria for this experiment required that the average insertion torque values for *Trabecular Metal* Implants were equivalent or fell between the maximum and minimum torque values exhibited by the control implants, and that the differences between test and control implants be statistically significant. Insertion torque values of the *Trabecular Metal* test implants ranged from a maximum 169.0Ncm (average = 161.1 ± 5.7Ncm) for 6.0mm x 13mm implants to a minimum of 100.5Ncm (average = 104.1 ± 3.8Ncm) for implants 4.7mm x 13mm (**Table 1**). Differences between the 4.7mmD test and 5.0mmD control implants were statistically significant. Average insertion torque data for 6.0mmD test and control implants were statistically equivalent.

*Trabecular Metal* Dental Implants exhibited insertion torque values within the range exhibited by the commercially available control implants. Numerous studies<sup>73-77</sup> have used insertion torque values as stability guidelines for determining whether a dental implant can sustain immediate loading, although there is no clinical consensus on what should constitute a minimum insertion torque level. In general, however, many clinicians<sup>73-77</sup> have selected an approximate insertion torque value of 35Ncm or greater as a determining guideline for immediate loading. The average insertion torque values of *Trabecular Metal* Material test implants in this study thus significantly exceeded this threshold (**Table 1**).

**Press-fit analysis of Trabecular Metal Dental Implants (ZRR-ZD-00064-00)** As compared to conventionally threaded implants, *Trabecular Metal* Implants have fewer external threads for primary stabilization, and a porous surface that forms a frictional interface with bone. This experiment evaluated the effect of torsional forces on the structural integrity of *Trabecular Metal* Dental Implants during and after placement in bone. Previous corporate experiments (ZRR-ZD-00060-00) assessed the amount of torque required to place solid *Trabecular Metal* Material cylinders into bone, and the result frictional placement had on the structural integrity of the material. Results provided baseline data for comparing results obtained when *Trabecular Metal* Material is incorporated into a threaded implant design. The amount of torque required to compromise the structural integrity of a *Trabecular Metal* Dental Implant was found to be significantly greater than the amount of torque actually placed on the *Trabecular Metal* Material itself during implant insertion into bone. Furthermore, a fully integrated implant was found to withstand a rotational force of greater than 355Ncm, which is more than 3-times greater than the anticipated worst-case torsional forces on molars during immediate occlusal loading (110Ncm, per Engineering Analysis, Lab notebook ZDI-269 pp. 28-31). These findings suggest that the *Trabecular Metal* Material region of the dental implant will not be structurally compromised by torsional forces during placement or immediate loading.

**Trabecular Metal Dental Implant placement utilizing soft bone and dense bone surgical protocols (ZRR-ZD-00076-00)** Implant placement in bone with moderate to high density (types 1 to 3)<sup>78</sup> utilizes a final step-drill that prepares a narrower diameter in the apical region of the osteotomy. This technique enables approximately one-third of a tapered implant design to enter the osteotomy before the self-tapping implant threads engage the walls of the receptor site, which may facilitate implant placement in sites with limited vertical access.<sup>79</sup> In low-density (type 4)<sup>78</sup> bone, final osteotomy preparation is performed with a straight drill that is 0.2mm to 0.3mm smaller than the apical end of a tapered implant, depending on the implant diameter.<sup>79</sup> This soft-bone surgical technique is designed to enable the tapered, apical end of an implant to laterally engage the osteotomy walls and gradually compress the surrounding bone to a maximum of 0.6mm or 0.7mm at the crest of the ridge, depending on the implant diameter.<sup>79</sup> When the diameter of an osteotomy is a minimum of 100µm smaller than that of the implant, force-fitting stresses generated during placement have been reported to increase placement torque and implant stability, as compared to implants not placed into smaller diameter osteotomies in low-density bone.<sup>79-81</sup>

The present experiment was primarily designed to determine if *Trabecular Metal* Dental Implants could be successfully placed in a surrogate soft bone substrate utilizing a soft bone surgical protocol. A second part to this experiment evaluated whether *Trabecular Metal* Dental Implants could also be placed into dense bone when a soft bone protocol was used. In this case, a successful test was



**Table 1. Insertion torque results (Ncm), \*=statistically equivalent**

NobelReplace Implant 5.0mm x 13mm	Trabecular Metal Implant		Tapered Screw-Vent Implant	
	4.7mm x 13mm	6.0mm x 13mm	6.0mm x 13mm	
84.5 Ncm	103.0	154.0	174.0	177.0
89.5 Ncm	103.0	169.0	160.5	174.0
95.0 Ncm	100.5	158.5	141.5	186.5
91.0 Ncm	103.5	164.0	146.0	131.0
87.5 Ncm	110.5	160.0	130.5	
<b>Min: 84.5</b> <b>Max: 95.0</b>	<b>Min: 100.5</b> <b>Max: 110.5</b>	<b>Min: 154</b> <b>Max: 169</b>	<b>Min: 130.5</b> <b>Max: 186.5</b>	
Avg: 89.5	Avg: 104.1	Avg: 161.1*	Avg: 157.9*	
Std Dev: 3.9	Std Dev: 3.8	Std Dev: 5.7	Std Dev: 21.2	

**Note:** Sample sizes determined based on part availability and requirement for normally distributed data.

classified as either full placement with a soft bone protocol, or subsequent dense bone protocol, if needed. Experiments showed that *Trabecular Metal* Implants could be optimally placed if the soft bone surgical protocol was used in soft bone, and the dense bone surgical protocol was used in all other bone densities.

#### Material analysis of Trabecular Metal Dental Implants following exposure to surface cleaning solutions (ZRR-ZD-00054-00)

This experiment evaluated the effect of cleaning materials used to remove hydroxylapatite residue following secondary grit-blasting. The contact materials consisted of 5% hydrochloride (HCl), distilled water, acetone, isopropyl alcohol (IPA), and sustained heat on *Trabecular Metal* Material cylinders. The impact of the contact materials on *Trabecular Metal* Material was analyzed by mechanical/chemical methods. Results of the analysis indicated that the *Trabecular Metal* Material cylinders did not suffer adverse effects from the production cleaning methods used in this experiment.

#### Evaluation of Trabecular Metal Dental Implants in the canine model

In 2009, researchers<sup>82</sup> from The Ohio State University and Zimmer Dental collaborated on the first *in vivo* study of a *Trabecular Metal* Dental Implant design. The objectives of the study were to investigate whether *Trabecular Metal* Material applied to a dental implant would osseointegrate.<sup>82</sup> A total of 24 experimental *Trabecular Metal* Implants were placed in mandibles of 8 dogs (3 implants per dog).<sup>82</sup> Additionally 24 control implants (*Tapered Screw-Vent* Implant, Zimmer Dental Inc.) were placed in the mandibles of the same 8 dogs (3 implants per dog).<sup>82</sup> Two (2) animals each were euthanized at 2, 4, 8 and 12 weeks after implantation.<sup>82</sup> Calcein was injected prior to necropsy to label newly mineralizing bone tissue.<sup>82</sup> Two histological sections from each implant were prepared: one section was used to assess the calcein-labeled tissue and the other was stained by Goldner's Trichrome to assess osteoid and matured bone.<sup>82</sup> Effects of healing time on the histomorphometric analysis measurements were statistically analyzed.<sup>82</sup>

At all time periods, average bone-to-implant contact (BIC) on the titanium alloy (i.e. non-*Trabecular Metal* Material) portions of the implants exceeded 70%. New bone formation inside *Trabecular Metal* Material pores was evident at 2 weeks and bone ingrowth across the full thickness of the porous surface was observed at 4 weeks.<sup>82</sup> Histomorphometric analyses of bone in *Trabecular Metal* Material pores indicated rapid bone fill and remodeling: 1) the highest amount of newly mineralizing tissue was observed at week 2 (36.08%) and significantly lower at later weeks (17.69%, 22.40% and 19.95% respectively,  $p < 0.05$ ) and 2) osteoid was highest at week 2 (63.53%) and significantly lower at weeks 8 and 12 (35.97% and 41.94%, respectively,  $p < 0.05$ ).<sup>82</sup> Matured bone significantly increased during the same time intervals (3.32%, 9.01% and 18.69% at 2, 8 and 12 weeks, respectively,  $p < 0.05$ ).<sup>82</sup> Active bone formation into the porous surface of *Trabecular Metal* Implants observed at the early healing stage supports its potential use in dental implant applications.<sup>82</sup> Unlike the experimental titanium fiber mesh implants previously cited,<sup>39-46</sup> the *Trabecular Metal* Implants in the present study did not exhibit fibrous tissue anywhere along the bone-implant interface or inside the *Trabecular Metal* Material pores.

#### Discussion

Early development and evaluations of *Trabecular Metal* Dental Implants have demonstrated their ability to adequately meet the biomechanical demands encountered in the dental environment and to biologically integrate in the canine model. How the material will function in human dental patients, especially when immediately loaded, will be the next research phase of *Trabecular Metal* Dental Implants. In 2010, Zimmer Dental established a prospective pilot clinical study of *Trabecular Metal* Dental Implants, and a multi-national *Trabecular Metal* Implant Longitudinal Data Collection Program that will continue to monitor and gather data on the implants over the coming years. New data will be published as it is accrued.

## References

- 1 Ring ME. A thousand years of dental implants: a definitive history — part 1. *Compend Contin Educ Dent*. 1995;16:1060,1062,1064 passim.
- 2 Ring ME. A thousand years of dental implants: a definitive history — part 2. *Compend Contin Educ Dent*. 1995;16:1132,1134,1136 passim.
- 3 Greenfield, EJ. Implantation of artificial crown and bridge abutments. *Dental Cosmos*. 1913;55:364-369.
- 4 Linkow LI, Rinaldi AW. Evolution of the Vent-Plant osseointegrated compatible implant system. *Int J Oral Maxillofac Implants*. 1988;3:109-122.
- 5 Grundschober F, Kellner G, Eschberger J, Plenk H Jr. Long term osseous anchorage of endosseous dental implants made of tantalum and titanium. In: Winter GB, Gibbons DF, Plenk H Jr (Eds.). *Biomaterials 1980*. Chichester: John Wiley & Sons, 1982:365-370.
- 6 Grenoble DE, Voss R. Analysis of five years of study of vitreous carbon endosseous implants in humans. *Oral Implantol*. 1977;6:509-525.
- 7 Grenoble DE, Voss R. Case studies with carbon endosseous implants. *Alpha Omegan*. 1975;68:16-19.
- 8 Lemons JE. Biomaterials science protocols for clinical investigations on porous alumina ceramic and vitreous carbon implant. *J Biomed Mater Res Symposium*. 1975;6:9-16.
- 9 Kawahara H, Hirabayashi M, Shikita T. Single crystal alumina for dental implants and bone screws. *J Biomed Mater Res*. 1980;14:597-605.
- 10 Arvidson K, Fartash B, Moberg L-E, Grafström R, Ericsson I. In vitro and in vivo experimental studies on single crystal sapphire dental implants. *Clin Oral Impl Res*. 1991;2:47-55.
- 11 Brånemark PI, Hansson BO, Adell R, Breine U, Lindström J, Hallén O, Öhman A. Osseointegrated implants in the treatment of the edentulous jaw. Experience from a 10-year period. *Scand J Plast Reconstr Surg*. 1977;111 (Suppl 16):1-132.
- 12 Brånemark PI. Osseointegration and its experimental background. *J Prosthet Dent*. 1983;50:399-410.
- 13 Brånemark PI. Introduction to osseointegration. In Brånemark PI, Zarb GA, and Albrektsson T (Eds.): *Tissue-Integrated Prostheses. Osseointegration in Clinical Dentistry*. Chicago, IL: Quintessence Publishing Co, Inc, 1985:11-76.
- 14 Brånemark PI. Tooth replacement by oral endoprostheses: Clinical aspects. *J Dent Educat*. 1988;52:821-823.
- 15 Bothe RT, Beaton LE, Davenport HA. Reaction of bone to multiple metallic implants. *Surg, Gynecology, and Obstetrics*. 1940;71:598-602.
- 16 Leventhal GS. Titanium, a metal for surgery. *J Bone Joint Surg*. 1951;33(A):473-474.
- 17 Clarke EGC, Hickman J. An investigation into the correlation between the electric and potential of metals and their behaviour in biological fluids. *J Bone Joint Surg*. 1953;35(B):467-473.
- 18 Brunski JB. Biomaterials and biomechanics in dental implant design. *Int J Oral Maxillofac Implants*. 1988;3(2):85-97.
- 19 Clark AE. Principles of tissue implant material interactions. In Caswell CW, Clark Jr. AE (Eds.): *Dental Implant Prosthodontics*. Philadelphia: JB Lippincott Co, 1991:317-322.
- 20 Williams DF. Titanium as a metal for implantation. Part I: Physical properties. *J Med Engineer Tech*. 1977;7:195-198, 202.
- 21 Wigfield C, Robertson J, Gill S, Nelson R. Clinical experience with porous tantalum cervical interbody implants in a prospective randomized controlled trial. *Br J Neurosurg*. 2003;17:418-425.
- 22 Hacking SA, Bobynd JD, Toh KK, Tanzer M, Krygier JJ. Fibrous tissue ingrowth and attachment to porous tantalum. *J Biomed Mater Res*. 2000;52:631-638.
- 23 Shimko DA, Shimko VF, Sander EA, Dickson KF, Nauman EA. Effect of porosity on the fluid flow characteristics and mechanical properties of tantalum scaffolds. *J Biomed Mater Res. Part B: Appl Biomater*. 2005;73B:315-325.
- 24 Nasser S, Poggie RA. Revision and salvage patellar arthroplasty using a porous tantalum implant. *J Arthroplasty*. 2004;19:562-572.
- 25 Tsao AK, Roberson JR, Christie MJ, Dore DD, Heck DA, Robertson DD, Poggie RA. Biomechanical and clinical evaluations of a porous tantalum implant for the treatment of early-stage osteonecrosis. *J Bone Joint Surg*. 2005;87-A(Suppl 2):22-27.
- 26 Unger AS, Lewis RJ, Gruen T. Evaluation of a porous tantalum uncemented acetabular cup in revision total hip arthroplasty. Clinical and radiological results of 60 hips. *J Arthroplasty*. 2005;20:1002-1009.
- 27 Zardiackas LD, Parsell DE, Dillion LD, Mitchell DW, Nunnery LA, Poggie R. Structure, metallurgy, and mechanical properties of a porous tantalum foam. *J Biomed Mater Res (Appl Biomater)*. 2001;58:180-187.
- 28 Bobynd JD, Stackpool GJ, Hacking SA, Tanser M, Krygier JJ. Characteristics of bone ingrowth and interface mechanics of a new porous tantalum biomaterial. *J Bone Joint Surg (Br)*. 1999;81-B:907-914.
- 29 Bobynd JD. UHMWPE: the good, bad & ugly. Fixation and bearing surfaces for the next millennium. *Orthop*. 1999;22:810-812.
- 30 Khurana JS, Fordyce H, Sidebotham C, Smith G. Bone growth in a novel osteoconductive material for artificial bone replacement. Submitted to the 45<sup>th</sup> Annual Meeting of the Orthopaedic Research Society, Anaheim, CA, USA, February 1-4, 1999.
- 31 Bobynd JD, Toh KK, Hacking A, Tanzer M, Krygier JJ. Tissue response to porous tantalum acetabular cups. *J Arthroplasty*. 1999;14:347-354.
- 32 Bobynd JD, Poggie RA, Krygier JJ, Lewallen DF, Hanssen AD, Lewis RJ, Unger AS, O'Keefe TJ, Christie MH, Nasser S, Wood JE, Stulberg SD, Tanzer M. A structural porous tantalum biomaterial for adult reconstruction. *J Bone Joint Surg*. 2004;86-A(Suppl 2):123-129.
- 33 Gruen TA, Poggie RA, Lewallen DF, Hanssen Ad, Lewis RJ, O'Keefe TJ, Stulberg SD, Suthreland CJ. Radiographic evaluation of a monoblock acetabular component. *J Arthroplasty*. 2005;20:369-378.
- 34 Nehme A, Lewallen DF, Hanssen AD. Modular porous metal augments for treatment of severe acetabular bone loss during revision hip arthroplasty. *Clin Orthop Relat Res*. 2004;429:201-208.
- 35 Kaplan RB, Smith GK, Khurana JS, Puerto DA, LaFond E, Sidebotham C. Mandibular reconstruction with a porous tantalum implant in a canine model. National Institutes of Health, Grant No. DE09781-03, 1997.
- 36 Smith GK, Fordyce HH, Puerto DA, Khurana J, Cohen R. Bone ingrowth and remodeling associated with Hydrocel canine mandibular reconstruction implant. Submitted to the 46<sup>th</sup> Annual Meeting of the Orthopaedic Research Society, Orlando, FL, USA, March 12-15, 2000.
- 37 Smith G, Poggie R, Fordyce H, Hosalkar H, Khurana J, Scherbel U, Schultz P, Sidebotham C, Cohen R. Characterization of bone ingrowth and remodeling in a canine mandibular defect model. Submitted to the 47<sup>th</sup> Annual Meeting of the Orthopaedic Research Society, San Francisco, CA, USA, February 25-28, 2001.
- 38 Dillion LD, Zardiackas LD. Mechanical integrity between Hydrocel and a single tooth implant. Presented at the Annual Research Meeting of the American Association for Dental Research, Chicago, Illinois, USA, March 2001.
- 39 Weiss MB. Development of an endosseous dental implant (I). *Quintessence Int Dent Dig*. 1977;8:87-91.
- 40 Weiss MB, Rostoker W. Development of an endosseous dental implant (II). *Quintessence Int Dent Dig*. 1977;8:107-112.
- 41 Weiss MB, Rostoker W. Development of an endosseous dental implant (III). *Quintessence Int Dent Dig*. 1977;8:77-84.
- 42 Weiss MB, Rostoker W. Development of an endosseous dental implant (IV). *Quintessence Int Dent Dig*. 1977;8:75-80.
- 43 Weiss MB, Rostoker W. Development of a new endosseous dental implant. Part I: animal studies. *J Prosthet Dent*. 1981;46:646-651.
- 44 Weiss MB, Rostoker W. Development of a new endosseous dental implant. Part II: human studies. *J Prosthet Dent*. 1982;47:633-645.
- 45 Weiss MB, Gutman D, Rostoker W. A new fiber metal dental implant. *Compend Contin Educ Dent*. 1984;5:383-388.
- 46 Weiss MB. Titanium fiber-mesh metal implant. *J Oral Implantol*. 1986;12:498-507.
- 47 Black J. Biological performance of tantalum. *Clin Mater*. 1994;16:167-173.
- 48 American Society for Testing and Materials. Standard specification for unalloyed tantalum for surgical implant applications (ASTM F 560-98). In: *Annual Book of ASTM Standards*, ASTM, 1998;13.01:63-65.
- 49 Koutostathis SD, Tsakotos GA, Papakostas I, Macheras GA. Biological process at bone-porous tantalum interface. A review article. *J Orthopaedics*. 2009;6(4)e3. Available online at <http://www.jortho.org/2009/6/4/e3>. Accessed 31 March 2010.
- 50 Plenk H Jr, Pfluger G, Schider S, Bohler N, Grundschober F. The current status of uncemented tantalum and niobium femoral endoprostheses. In: Morscher E (Ed.): *The Cementless Fixation of Hip Endoprostheses*. Berlin: Springer-Verlag, 1984:174-177.
- 51 Brown MA, Carden JA, Coleman RE, McKinney R Jr., Spicer LD. Magnetic field effects on surgical ligation clips. *Magn Reson Imaging*. 1987;5:443-453.
- 52 Pudenz RH. The repair of cranial defects with tantalum: an experimental study. *J Amer Med Assoc*. 1943;121:478-481.
- 53 Echols DH, Colclough JA. Cranioplasty with tantalum plate. Report of eight cases. *Surgery. A Monthly Journal Devoted to the Art and Science of Surgery*. 1945;17:304-414.
- 54 Bellinger DH. Preliminary report on the use of tantalum maxillofacial and oral surgery. *J Oral Surg*. 1947;5:108-122.
- 55 Spurling RG. The use of tantalum wire and foil in the repair of peripheral nerves. *Surg Clin North Am*. 1943;23:1491-1504.
- 56 McFadden JT. Tissue reactions to standard neurosurgical metallic implants. *J Neurosurg*. 1972;36:598-603.

- <sup>57</sup> Johnson PF, Bernstein JJ, Hunter G, Dawson WW, Hench LL. An in vitro and in vivo analysis of anodized tantalum capacitive electrodes: corrosion response, physiology and histology. *J Biomed Mater Res.* 1977;11:637-656.
- <sup>58</sup> McClung EJ, Chipps JE. Tantalum foil used in closing antro-oral fistulas. *US Armed Forces Med J.* 1951;2:1183-1186.
- <sup>59</sup> Aronson AS, Jonsson N, Alberius P. Tantalum markers in radiography: an assessment of tissue reactions. *Skeletal Radiol.* 1985;14:207-211.
- <sup>60</sup> Burke GL. The corrosion of metals in tissues and an introduction to tantalum. *Can Med Assoc J.* 1940;43:125-128.
- <sup>61</sup> Kokubo T. Metallic materials stimulating bone formation. *Med J Malaysia.* 2004;59(Suppl B):91-92.
- <sup>62</sup> Findlay DM, Welldon K, Atkins GJ, Howie DW, Zannettino AC, Bobyn D. The proliferation and phenotypic expression of human osteoblasts on tantalum metal. *Biomaterials.* 2004;25:2215-2227.
- <sup>63</sup> Welldon KJ, Atkins GJ, Howie DW, Findlay DM. Primary human osteoblasts grow into porous tantalum and maintain an osteoblastic phenotype. *J Biomed Mater Res A.* 2008;84(3):691-701.
- <sup>64</sup> Benson J. Elemental carbon as a bio-material. *J Biomed Mater Res.* 1971;5:41-47.
- <sup>65</sup> Kadefors R, Martin RI, Reswick JB. A percutaneous electrode for long-term monitoring of bio-electrical signals in humans. *Med Biol Eng.* 1970;8:129-135.
- <sup>66</sup> Markle DH, Grenoble DE, Melrose RJ. Histologic evaluation of vitreous carbon endosteal implants in dogs. *Biomater Med Devices Artif Organs.* 1975;3:97-114.
- <sup>67</sup> Cowland FC, Lewis JC. Vitreous carbon—a new form of carbon. *J Mat Sci.* 1967;2:507-512.
- <sup>68</sup> Stanitski CL, Mooney V. Osseous attachment to vitreous carbons. *J Biomed Mater Res Symposium.* 1973;4:97-108.
- <sup>69</sup> Anusavice KJ. *Phillips' Science of Dental Materials (Anusavice Phillip's Science of Dental Materials)*. 11<sup>th</sup> ed. Philadelphia: Saunders Publishing, 2003.
- <sup>70</sup> International Organization for Standardization. *Dentistry – Implants – Dynamic Fatigue Test for Endosseous Dental Implants (ISO 14801)*. Available online at: [http://www.iso.org/iso/iso\\_catalogue.htm](http://www.iso.org/iso/iso_catalogue.htm). Accessed 1 April 2010.
- <sup>71</sup> Ormianer Z, Palti A. Retrospective clinical evaluation of Tapered Screw-Vent implants: results after up to eight years of clinical function. *J Oral Implantol.* 2008;34:150-160.
- <sup>72</sup> Lee CYS, Rohrer MD, Prasad HA. Immediate loading of the grafted maxillary sinus using platelet rich plasma and autogenous bone: a preliminary study with histologic and histomorphometric analysis. *Implant Dent.* 2008;17:59-73.
- <sup>73</sup> Ostman PO, Hellman M, Sennerby L. Direct implant loading in the edentulous maxilla using a bone density-adapted surgical protocol and primary implant stability criteria for inclusion. *Clin Implant Dent Relat Res.* 2005;7:S60-S69.
- <sup>74</sup> Fischer K, Bäckström M, Sennerby L. Immediate and early loading of oxidized tapered implants in the partially edentulous maxilla: a 1-year prospective, clinical, radiographic, and resonance frequency analysis study. *Clin Implant Dent Relat Res.* 2009;11:69-80.
- <sup>75</sup> Neugebauer J, Weinländer M, Lekovic V, von Berg KH, Zoeller JE. Mechanical stability of immediately loaded implants with various surfaces and designs: a pilot study in dogs. *Int J Oral Maxillofac Implants.* 2009;24:1083-1092.
- <sup>76</sup> Hui E, Chow J, Li D, Liu J, Wat P, Law H. Immediate provisional for single-tooth implant replacement with a Brånemark system: preliminary report. *Clin Implant Dent Relat Res.* 2001;3:79-82.
- <sup>77</sup> Achilli A, Tura F, Euwe E. Immediate/early function with tapered implants supporting maxillary and mandibular posterior fixed partial dentures: preliminary results of a prospective multicenter study. *J Prosthet Dent.* 2007;97:S52-S58.
- <sup>78</sup> Calandriello R, Tomatis M, Rangert B. Immediate functional loading of Brånemark System implants with enhanced initial stability: a prospective 1- to 2-year clinical and radiographic study. *Clin Implant Dent Relat Res.* 2003;5:10-20.
- <sup>79</sup> Cannizzaro G, Torchio C, Leone M, Esposito M. Immediate versus early loading of flapless-placed implants supporting maxillary full-arch prostheses: a randomised controlled clinical trial. *Eur J Oral Implantol.* 2008;1:127-139.
- <sup>80</sup> Anusavice KJ. *Phillips' Science of Dental Materials (Anusavice Phillip's Science of Dental Materials)*. 11<sup>th</sup> ed. Philadelphia: Saunders Publishing, 2003.
- <sup>81</sup> International Organization for Standardization. *Dentistry – Implants – Dynamic Fatigue Test for Endosseous Dental Implants (ISO 14801)*. Available online at: [http://www.iso.org/iso/iso\\_catalogue.htm](http://www.iso.org/iso/iso_catalogue.htm). Accessed 1 April 2010.
- <sup>82</sup> Lekholm U, Zarb GA. Patient selection and preparation. In: Brånemark PI, Zarb GA, Albrektsson T (Eds.): *Tissue-Integrated Prostheses. Osseointegration in Clinical Dentistry*. Chapter 12. Chicago: Quintessence Books, 1985:199-209.
- <sup>83</sup> Le Gall MG. Localized sinus elevation and osteocompression with single-stage tapered dental implants: technical note. *Int J Oral Maxillofac Implants.* 2004;19:431-437.
- <sup>84</sup> Skalak R, Zhao Y. Interaction of force-fitting and surface roughness of implants. *Clin Implant Dent Relat Res.* 2000;2:219-234.
- <sup>85</sup> Callan DP, Hahn J, Hebel K, Kwong-Hing A, Smiler D, Vassos DM, Wöhrle P, Zosky J. Retrospective multicenter study of an anodized, tapered, diminishing thread implant: success rate at exposure. *Implant Dent.* 2000;9:329-336.
- <sup>86</sup> Kim D-G, Huja SS, Larsen PE, Kreuter KS, Chien H-H, Joo W, Wen HB. Trabecular Metal dental implants in an animal model. Abstract No. 1511. Presented at the Annual Meeting of the American Association for Dental Research, Washington, DC, USA, March 3-6, 2010.